

◆ PRECISION INSTRUMENTS FOR TEST AND MEASUREMENT ◆

HACS-Z-A-7E-1pF

Decade Capacitance System User and Service Manual



Copyright © 2010 IET Labs, Inc.
Visit www.ietlabs.com for manual revision updates

HACS-Z-A-7E-1pF im/April 2010



IET LABS, INC.

Long Island, NY • Email: info@ietlabs.com

www.ietlabs.com
TEL: (516) 334-5959 • (800) 899-8438 • FAX: (516) 334-5988

◆ PRECISION INSTRUMENTS FOR TEST AND MEASUREMENT ◆



IET LABS, INC.

Long Island, NY • Email: info@ietlabs.com

www.ietlabs.com

TEL: (516) 334-5959 • (800) 899-8438 • FAX: (516) 334-5988

Contents

Chapter 1 Introduction	1
1.1 General Description	1
1.2 Switches	2
1.3 Double Shielded Construction	2
Chapter 2 Specifications	3
Specifications	3
Double Shielded Construction	3
Chapter 3 Operation	5
3.1 Initial Inspection and Setup	5
3.2 Switch Setting	5
3.3 Connection to Terminals	5
Chapter 4	
Maintenance	7
4.1 Preventive Maintenance	7
4.2 Calibration Interval	7
4.3 Considerations for Calibration	7
4.4 Calibration Procedure	8
4.5 Capacitance Adjustment	8
4.5.1 Adjusting 1 pF - 1,000 pF decades	8
4.5.2 Adjusting 0.01 μ F - 1 μ F decades	9
4.6 Replaceable Parts	10

Figures and Tables

Figure 1-1: <i>HACS-Z-7E-1pF</i>	1
<i>Figure 1-2: Capacitance Shunted by Leakage to case</i>	2
<i>Figure 1-3: HACS-Z Construction</i>	2
<i>Table 2-1: Specifications</i>	3
<i>Figure 2-1: Double Shielded Construction</i>	3
<i>Figure 2-2: Typical Operating Guide Affixed to HACS-Z-7E-1pF</i>	4
<i>Figure 3-1: Capacitance Shunted by Leakage to case</i>	5
<i>Figure 3-2: HACS-Z Construction</i>	6
<i>Table 4-1: Capacitor type</i>	8
<i>Figure 4-1: Calibration access holes</i>	8
<i>Figure 4-2: Screws holding the internal housings</i>	9
<i>Figure 4-3: 0.01 μF & 0.1 μF capacitance sets</i>	9
<i>Figure 4-4: 1μF Capacitance Set</i>	9
<i>Table 4-2: Replaceable Parts List</i>	10
<i>Figure 4-5: Replaceable Parts</i>	10

Chapter 1

INTRODUCTION

1.1 General Description

The HACS-Z-7E-1pF Decade Capacitance System is capable of meeting exacting requirements for fixed or adjustable calibration capacitance or any applications requiring precise stable capacitance values.

Unit Features:

- Range: 1 pF - 11.111 11 μ F
- Low zero-capacitance
- High accuracy
- Excellent stability
- Low temperature coefficient
- High voltage rating



Figure 1-1: HACS-Z-7E-1pF

1 pF, 10 pF decades

For these, the lowest decade steps, trimmable air capacitors are used. The capacitors are selected for maximum resolution, high mechanical stability, and low dissipation factor.

100 pF - 0.1 μ F decades

These mid-range decades are implemented with the highest grade, mechanically stabilized, sealed India ruby mica capacitors selected for optimum electrical characteristics and low dissipation. They are hermetically sealed to prevent intrusion of moisture and to obtain minimum drift.

1 μ F decade

This decade is implemented with metallized polyphenylene sulfide (MPPS). These capacitors are hermetically sealed for high reliability and stability. Hermetic sealing prevents the intrusion of moisture into the capacitor packages, and results in minimum drift.

Stability

The stability of the capacitors is such that the instrument should not require readjustment for the duration of the recommended calibration interval. Should recalibration become necessary, easily accessible trimmer capacitors are provided for the 1 pF, 10 pF, 100 pF, and 1000 pF decades. The other decades may also be calibrated with discrete pad-der capacitors.

1.2 Switches

Custom-designed switches are used to connect four capacitors in a parallel circuit for each decade. These are weighted in a 1-2-2-5 code to provide all the necessary combinations for ten equal steps for each decade.

The switch circuit is designed such that each unused capacitor is completely disconnected from the rest of the circuit and has its positive terminal connected to the inner shield. See Figure 1-3.

The stability of the switches is assured by the use of large gaps and secure mechanical construction.

1.3 Double Shielded Construction

In order to meet the low residual capacitance requirement, the unit utilizes:

- Specially shielded and routed wiring
- The switching scheme described above and shown in Figure 1-2
- A double-shielded construction to keep the zero capacitance at an extremely low level

Figure 1-2 demonstrates the need for the double shielded construction. It shows that a capacitor C_{HL} would be shunted by the series combination of the capacitances from the HIGH and LOW terminals to the case. The net capacitance becomes:

$$C_{HL} + (C_{HG} \text{ in series with } C_{LG})$$

Clearly it would be very difficult to get a very low residual or zero capacitance, unless the G terminal is the ground terminal of 3-terminal measurement of the capacitance.

In order to accomplish this, an inner shield is added as conceptually shown in Figure 1-3. It is mechanically constructed to shunt away any capacitance between the HIGH and LOW terminals.

shield shunts this capacitance when it is electrically connected to the outer shield, forming a 3-terminal capacitor (5-terminal capacitor for units with 10 μF steps or higher). All unused capacitors are shorted to this inner shield at their high ends, and are open at their low ends.

This inner shield is not actually an internal enclosure but rather a cellular structure that optimally separates all conductors and capacitor elements. It also serves to minimize terminal-to-ground capacitance which is necessary when measuring small capacitances with various bridges.

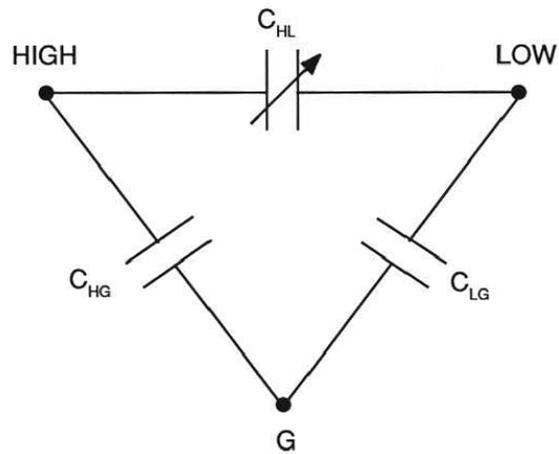


Figure 1-2: Capacitance Shunted by Leakage to case

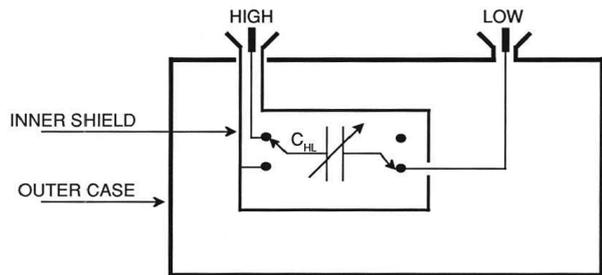


Figure 1-3: HACS-Z Construction

Chapter 2

SPECIFICATIONS

For convenience to the user, the pertinent specifications are given in an **Operating Guide**, similar to the one shown in Figure 2-2, which is affixed to the case of the instrument.

SPECIFICATIONS

Capacitance per step	Total decade capacitance	Max voltage	Accuracy*	Dissipation factor*	Stability	Capacitor type
1 pF	10 pF	500 V peak max up to 10 kHz	$\pm (0.05\% + 0.5 \text{ pF})$	<0.002	$\pm(200 \text{ ppm} + 0.1 \text{ pF})$ per year	Air capacitors
1 pF	100 pF			Position 1: <0.002 All others: <0.001		
100 pF	1 nF			Position 1: <0.001 Position 2: <0.0005 All others: <0.0003		
1,000 pF	10 nF			<0.0003		
0.01 μF	100 nF			<0.0003		
0.1 μF	1 μF		<0.0004			Silvered mica Mechanically stabilized Hermetically sealed
1 μF	10 μF	50 V peak max		<0.0010	$\pm 500 \text{ ppm per year}$	Sealed metallized polyphenylene sulfide (MPPS)

*Bottom terminals for **all decades**

1 kHz, 3-terminal measurement; series model; 1 Vrms, 23°C; traceable to SI

No zero-subtraction required

Table 2-1: Specifications

Range:

0 to 11.111 110 μF , in 1 pF steps

Zero Capacitance:

$\leq 0.1 \text{ pF}$ maximum capacitance obtained with all dials set to zero;

Temperature Coefficient:

1 pF - 0.1 μF decades: $\approx 20 \text{ ppm}/^\circ\text{C}$

1 μF decade: $-50 \text{ ppm}/^\circ\text{C}$

Insulation Resistance:

$> 50,000 \text{ M}\Omega$

Operating Temperature Range:

10°C to 40°C

Shielding:

Double-shielded construction; see below.

Dimensions:

54 cm W x 32 cm H x 33 cm D (21" x 12.5" x 13")

Weight:

23 kg (51 lbs)

Connection to Capacitor:

Four bnc connectors labeled **HI** and **LO** located on the front. The shielding is divided into the following parts:

The inner shield: minimizes the terminal-to-guard capacitance

Outer shield (the case): minimizes the detector input capacitance and noise

The outer shells of the **HI** connectors are connected to the switch shaft. The outer shells of the **LO** connectors are connected to the outer case. To use the HACS-Z as a 3-terminal capacitance substituter with very low zero-capacitance connect the two shields together at the measuring instrument.

DOUBLE SHIELDED CONSTRUCTION

The shielding is divided into two different parts: an inner shield that minimizes the low terminal-to-guard capacitance, and an outer shield (the case) that minimizes the detector input capacitance and noise. (See Figure 2-1.)

When these two shields are connected together, the HACS-Z becomes an excellent 3-terminal capacitance substituter with low zero capacitance.

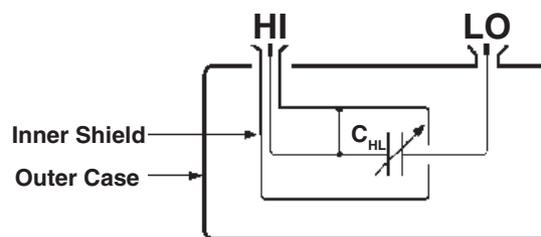


Figure 2-1: Double Shielded Construction

HACS-Z-A-7E-1pF HIGH ACCURACY DECADE CAPACITANCE SUBSTITUTER

CONSULT INSTRUCTION MANUAL FOR PROPER INSTRUMENT OPERATION

Range:
0 to 1,111,10 μF , in 1 pF steps

Zero capacitance:
<0.1 pF maximum capacitance obtained when all dials are set to zero

Temperature coefficient:
 $\approx 20 \text{ ppm}/^\circ\text{C}$

Insulation resistance:
>50,000 M Ω

Operating temperature range:
10 $^\circ\text{C}$ to 40 $^\circ\text{C}$

Capacitance per step	Total decade capacitance	Max voltage	Accuracy*	Dispitation factor**	Stability	Capacitor type	
1 pF	10 pF	500 V peak max up to 10 kHz	$\pm(0.05\%+0.5 \text{ pF})$	<0.002 Position 1: <0.002 All others: <0.001 Position 1: <0.001 Position 2: <0.0005 All others: <0.0003	$\pm(200 \text{ ppm} + 0.1 \text{ pF})$ per year	Silvered mica Mechanically stabilized Hermetically sealed	
10 pF	100 pF						Air capacitors
100 pF	1 nF						
1,000 pF	10 nF						
0.01 μF	100 nF						
0.1 μF	1 μF	50 V peak max		<0.0004		Sealed metalized polyphenylene sulfide (M.P.P.S)	
1 μF	10 μF		<0.0010				

* 1kHz, 3-terminal measurement; series model; 1 Vrms; traceable to SI
No zero subtraction required

Connection to capacitor:

Two bnc connectors labeled **HI** and **LO** are located on the front panel. The shielding is divided into the following parts:
The inner shield: minimizes the terminal-to-guard capacitance
The outer shield (the case): minimizes the detector input capacitance and noise

The outer shell of the **HI** connector is connected to the switch shaft. The outer shell of the **LO** connector is connected to the outer case. To make the HACS-Z a 3-terminal capacitance substituter with very low zero-capacitance, connect these two shields together at the measuring instrument

MODEL: HACS-Z-A-7E-1pF SN: H1-1015332

WARNING

Observe all safety rules when working with high voltages or line voltages. Connect the (G) terminal to earth ground in order to maintain the case at a safe voltage. Whenever hazardous voltages (>45 V) are used, take all measures to avoid accidental contact with any live components: a) Use maximum insulation and minimize the use of bare conductors. b) Remove power when adjusting switches. c) Post warning signs and keep personnel safely away.



IET LABS, INC. • 534 Main Street, Westbury, NY 11590 • (516) 334-5959 • Fax: (516) 334-5988

CAGE CODE: 62015

www.ietlabs.com

HACS-ZIBsp1/HACS-Z-B-6E-1pF-TMDE/06-16-09/80%

Figure 2-2: Typical Operating Guide Affixed to HACS-Z-7E-1pF

Chapter 3

OPERATION

3.1 Initial Inspection and Setup

This instrument was carefully inspected before shipment. It should be in proper electrical and mechanical order upon receipt.

An **OPERATING GUIDE**, shown in Figure 2-2, is attached to the case of the instrument to provide ready reference to specifications.

3.2 Switch Setting

The HACS-Z Precision Capacitor has six capacitance decades. The actual capacitance for each decade is the product of the switch setting and the **CAPACITANCE PER STEP** indicated below each switch on the front panel.

Note, however, that if any dial is set on 10, a 1 is added to the next decade. For example, if the dials are set: to 10-9-9-10-1-1, the resultant capacitance is:

$$\begin{array}{r}
 1 \\
 1 \\
 10 \\
 9 \\
 9 \\
 \hline
 10 \\
 \text{Total } 1100011 \text{ pF}
 \end{array}$$

The zero capacitance of the **HACS-Z** unit is very low, but all settings are adjusted to accurately provide their nominal values, and it is *not necessary* to subtract the zero capacitance from any particular setting

3.3 Connection to Terminals

In order to properly use the HACS-Z capacitor, it is necessary to understand the use and function of each of the capacitor terminals. Refer to Figure 3-1 and note that a basic capacitor is a 2-terminal capacitor shown as C_{HL} . As described above, C_{HG} and C_{LG} , the capacitances to the case add to the capacitor C_{HL} unless the 3rd terminal G is connected to the guard of the measuring instrument.

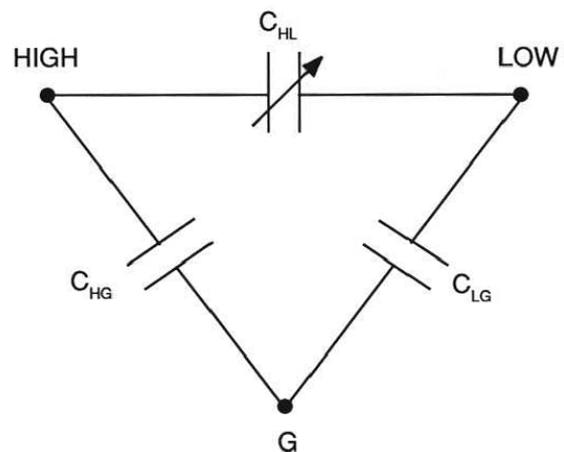


Figure 3-1: Capacitance Shunted by Leakage to case

The shielding is divided into two different parts: an inner shield that minimizes the low terminal-to-guard capacitance, and an outer shield (the case) that minimizes the detector input capacitance and noise. See figure 3-2.

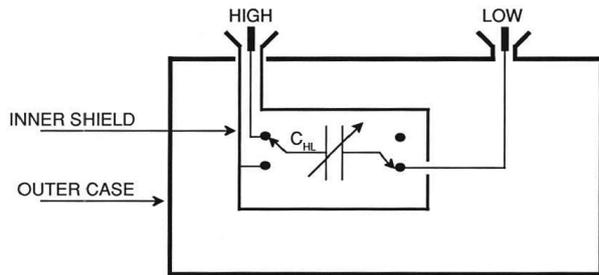


Figure 3-2: HACS-Z Construction

When these two shields are connected together, the HACS-Z becomes an excellent 3-terminal capacitance substituter with low zero capacitance.

Using the unit as a 2-terminal capacitor will cause an error of about 100 to 150 pF to be added. This error is not necessarily the same for every setting. This also makes the unit susceptible to noise. However, for high capacitance, the unit *may* be used as a 2-terminal device.

Chapter 4

MAINTENANCE

4.1 Preventive Maintenance

Keep the unit in a clean environment. This will help prevent possible contamination.

The HACS-Z is packaged in a closed case, which limits the entry of contaminants and dust into the instrument. If it is maintained in a clean or air-conditioned environment, cleaning will seldom be required. In a contaminated atmosphere, cleaning may be required.

To clean the front panel, wipe the front panel using alcohol and a lint-free cloth.

4.2 Calibration Interval

The recommended calibration interval for the **HACS-Z Capacitance Substituter** is twelve (12) months. The calibration procedure may be carried out by the user if a calibration capability is available, by IET Labs, or by a certified calibration laboratory.

If the user should choose to perform this procedure, then the considerations below should be observed.

4.3 Considerations for Calibration

It is important, whenever calibrating the HACS-Z unit, to be very aware of the capabilities and limitations of the test instruments used.

Recommended Instruments:

- **IET Model 1689 Digibridge** (direct reading)
or
- **IET Model 1620 or 1621 Precision Capacitance Measurement System** (bridge)

The test instruments must be significantly more accurate than $\pm(0.05\% + 0.5 \text{ pF})$ for all ranges, allowing for a band of uncertainty of the instrument itself.

It is important to allow both the testing instrument and the **HACS-Z** to stabilize for a number of hours at the nominal operating temperature of 23°C, and at nominal laboratory conditions of humidity. There should be no temperature gradients across the unit under test.

BNC test terminals should be used to obtain accurate shielded readings.

4.6 Replaceable Parts

Model Ref	IET Pt No	Description
1	0505-4030	Mica Capacitor, 100 pF
1	0505-4031	Mica Capacitor, 200 pF
1	0505-4032	Mica Capacitor, 500 pF
1	0505-4033	Mica Capacitor, 1 nF
1	0505-4034	Mica Capacitor, 2 nF
1	0505-4035	Mica Capacitor, 5 nF
1	0505-4036	Mica Capacitor, 10 nF
1	0505-4037	Mica Capacitor, 20 nF
1	0505-4038	Mica Capacitor, 50 nF
1	0505-4039	Mica Capacitor, 100 nF
1	0505-4040	Mica Capacitor, 200 nF
1	0505-4041	Mica Capacitor, 500 nF
2	4380-3700	Air Capacitor, 2.7-19.6 pF
3	4380-3600	Air Capacitor, 1.7-8.7 pF
4	4380-3500	Air Capacitor, 1.5-5.0 pF
5	HACS-Z-520033	Switch Assembly
6	HACS-Z-4300-KNB	Knob Assembly
Not Visible	HACS-Z-1μF	1 μF assembly
Not Visible	HACS-Z-PE4091	HIGH bnc connector
Not Visible	HACS-Z-31-221-RFX	LOW bnc connector
Not Visible	1413-BC-14215	Bail assembly

Table 4-2: Replaceable Parts List

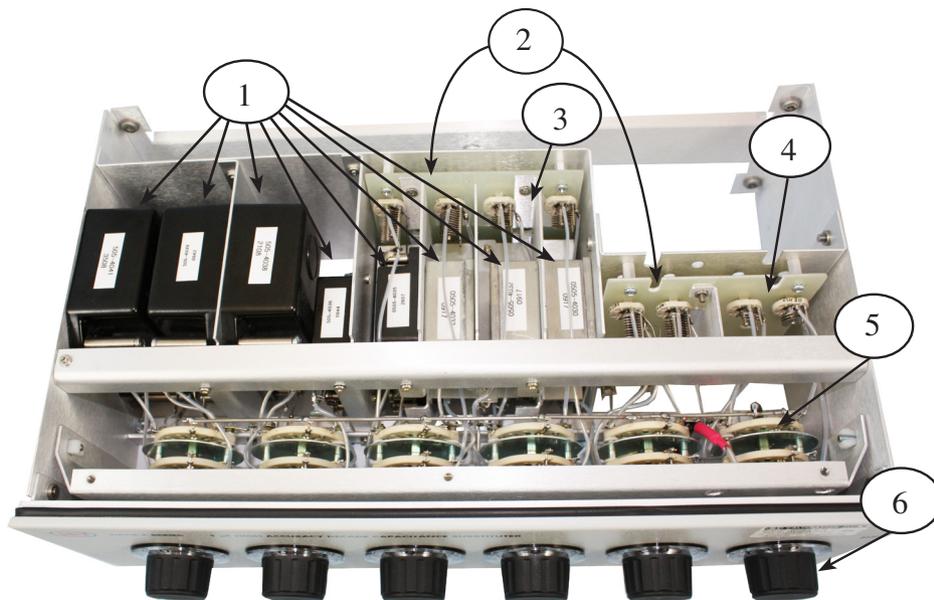


Figure 4-5: Replaceable Parts

