

◆ PRECISION INSTRUMENTS FOR TEST AND MEASUREMENT ◆

R-X SERIES
Decade Resistor
User and Service Manual



Copyright © 2002 IET Labs, Inc.

Effectivity: Serial Numbers beginning with P2
RX im/August, 2002



IET LABS, INC.

534 Main Street, Westbury, NY 11590

www.ietlabs.com
TEL: (516) 334-5959 • (800) 899-8438 • FAX: (516) 334-5988

WARRANTY

We warrant that this product is free from defects in material and workmanship and, when properly used, will perform in accordance with applicable IET specifications. If within one year after original shipment, it is found not to meet this standard, it will be repaired or, at the option of IET, replaced at no charge when returned to IET. Changes in this product not approved by IET or application of voltages or currents greater than those allowed by the specifications shall void this warranty. IET shall not be liable for any indirect, special, or consequential damages, even if notice has been given to the possibility of such damages.

THIS WARRANTY IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESSED OR IMPLIED, INCLUDING BUT NOT LIMITED TO, ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR ANY PARTICULAR PURPOSE.

Contents

WARRANTY	iii
Contents	iv
Figures	iv
WARNING	vi
CAUTION	vi
Chapter 1	
INTRODUCTION	1
Chapter 2	
SPECIFICATIONS	2
Chapter 3	
OPERATION	4
3.1 Initial Inspection and Setup	4
3.2. Connection	4
3.2.1 General Considerations	4
3.2.2 Electrical Considerations	4
3.2.3 Four-Wire Kelvin Lead Connections	4
3.2.4 Thermal emf Considerations	5
3.3 Dial Setting	5
3.4 Environmental Conditions	5
Chapter 4	
MAINTENANCE	6
4.1 Verification of Performance	6
4.1.1 Calibration Interval	6
4.1.2 General Considerations	6
4.1.3 Initial Procedure	6
4.1.4 Trimming Procedure	7
4.1.5 Repackaging for Shipment	7
4.1.6 Storage	7

Figures

Figure 1.1 RX Series High-Accuracy Decade Resistor	1
Figure 2.1 Typical Operating Guide Affixed to Unit	3
Figure 3.1 Optimal 4-Wire Kelvin Lead Connection	5



WARNING



OBSERVE ALL SAFETY RULES
WHEN WORKING WITH HIGH VOLTAGES OR LINE VOLTAGES.

ELECTRICAL SHOCK HAZARD. DO NOT OPEN CASE.
REFER SERVICING TO QUALIFIED PERSONNEL.

HIGH VOLTAGE MAY BE PRESENT WITH HIGH VOLTAGE OPTIONS.

WHENEVER HAZARDOUS VOLTAGES (> 45 V) ARE USED, TAKE ALL MEASURES TO
AVOID ACCIDENTAL CONTACT WITH ANY LIVE COMPONENTS:

- USE MAXIMUM INSULATION AND MINIMIZE THE USE OF BARE CONDUCTORS.

REMOVE POWER WHEN HANDLING UNIT.

POST WARNING SIGNS AND KEEP PERSONNEL SAFELY AWAY.



CAUTION



DO NOT APPLY ANY VOLTAGES OR CURRENTS TO THE TERMINALS OF THIS
INSTRUMENT IN EXCESS OF THE MAXIMUM LIMITS INDICATED ON
THE FRONT PANEL OR THE OPERATING GUIDE LABEL.

Chapter 1

INTRODUCTION

The **RX** Series of High-Accuracy Decade Resistors is a family of instruments providing a broad range of high-performance resistance sources. Any number of decades from three to seven is available, with steps of 1 m Ω to 1 M Ω .

The **RX** Series is a precision resistance source with excellent characteristics of stability, temperature coefficient, power coefficient, and frequency response.

The **RX** Series employs very-low-resistance switches with fine-silver contacts and fine-silver alloy wipers. A special design keeps zero resistance to less than 2 m Ω per decade. Self cleaning keeps the silver contacts from becoming tarnished when unused, or when only low currents are passed through them. This is most often the case when only minute test currents are drawn by digital multimeters or other test instruments. Contact resistance is stable and remains low and repeatable.

High-quality gold-plated tellurium-copper binding posts serve to minimize the thermal emf effects which would artificially reflect a change in dc resistance measurements. All other conductors within the instrument, as well as the solder employed, contain no metals or junc-

tions that could contribute to thermal emf problems.

The standard models offer a choice of three through seven decades. The panels are clearly labeled showing the step size and maximum current for each decade.

With a resolution as low as 1 m Ω and a maximum available resistance of over 11 M Ω , the **RX** Series may be used for exacting precision measurement applications requiring high accuracy, good stability, and low zero-resistance. They can be used as components of dc and ac bridges, for calibration, as transfer standards, and as RTD simulators.

The **RX** Series may be rack-mounted to serve as components in measurement and control systems.

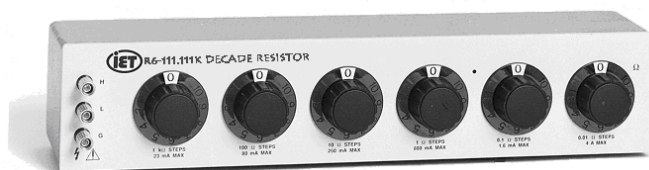


Figure 1.1. RX Series High-Accuracy Decade Resistor

Chapter 2

SPECIFICATIONS

For convenience to the user, the pertinent specifications are given in an **OPERATING GUIDE** affixed to the case of the instrument. Figure 2.1 shows a typical example.

SPECIFICATIONS

Model number code:

The digit following the letter “R” represents the number of decades. The number after the hyphen represents the full-scale resistance (with all switches set to ten) in ohms. A “K” denotes kilohms. A suffix “RC” indicates that the unit is equipped with angles for 19-inch relay-rack mounting.

Example: R7-111.1111K-RC is a seven decade rack-mounting unit with 111.1111K (111,111.11 ohms) with all switches set to ten. It is possible to set the box to higher resistance values by setting switches to eleven, instead of ten, but the total resistance value must then be calculated by adding the values set for the individual decades, which is time-consuming and can lead to errors.

Resistance per Step	Total Decade Resistance	Stability (±ppm/year)	Long Term Stability (±ppm/3 years)	Temperature Coefficient (±ppm/°C)	Max. Power (W/step)	Maximum current (per decade)	Maximum voltage (per step)
1 mΩ	10 mΩ	100	700	50	0.025	5 A	5 mV
10 mΩ	100 mΩ	50	350	20	0.2	4 A	40 mV
100 mΩ	1 Ω	30	50	20	0.25	1.6 A	0.16 V
1 Ω	10 Ω	10	25	20	0.6	0.8 A	0.8 V
10 Ω	100 Ω	10	25	15	0.6	0.25 A	2.5 V
100 Ω	1 kΩ	10	25	5	0.6	80 mA	8 V
1 kΩ	10 kΩ	10	25	5	0.5	23 mA	23 V
10 kΩ	100 kΩ	10	25	5	0.5	7 mA	70 V
100 kΩ	1 MΩ	10	25	5	0.5*	2.3* mA	230 V*
1 MΩ	10 MΩ	10	25	10	0.5*	0.7* mA	700 V*

*Subject to maximum of 2000 V.

Accuracy: After subtraction of zero resistance, at 23°C; traceable to NIST: ±(0.01% + 2 mΩ).

Zero Resistance: <2 mΩ per decade, at dc.

Maximum Voltage to Case: 1000 V peak.

Switch Type: 11 positions; "0"-10"; solid silver contacts and silver-alloy wipers.

Switch Capacitance: <0.15 pF per switch, low-loss.

Terminals: Low-thermal-emf beryllium-copper binding posts with standard 3/4 inch spacing, plus shield terminal.

Mechanical:

Model	Dimensions	Weight
3-4 decades	37.5 cm W x 8.9 cm H x 10.2 cm D (14.8" x 3.5" x 4")	1.7 kg (3.8 lb)
5 decades	43.9 cm W x 8.9 cm H x 10.2 cm D (17.3" x 3.5" x 4")	2.0 kg (4.3 lb)
6 decades		2.2 kg (4.8 lb)
7 decades		2.4 kg (5.3 lb)

Chapter 3

OPERATION

3.1 Initial Inspection and Setup

This instrument was carefully inspected before shipment. It should be in proper electrical and mechanical order upon receipt.

An **OPERATING GUIDE** is attached to the case of the instrument to provide ready reference to specifications.

3.2 Connection

3.2.1 General Considerations

The **RX Series Decade Resistors** provides three terminals labeled **H** (high), **L** (low), and **G** (ground). The **H** and **L** terminals are connected to the ends of the resistance being set; the **G** terminal is connected to the case. The **G** terminal may be used as a guard or shield terminal. It may also be connected (using a shorting link) to the **L** terminal to allow two-terminal as opposed to three-terminal measurements.

In order to make the most stable measurements, determine which is the more sensitive of the two user leads, i.e. the one going into a higher impedance. This lead should be connected to the more protected one of the two **RX** terminals. That would either be the **RX** terminal that is shorted to the case, or the **L** terminal when neither is connected to the case.

3.2.2 Electrical Considerations

In order to make proper use of the full performance capabilities of the **RX** unit, especially if low resistance values or low-resistance increments are important, care must be taken in connecting to its terminals.

In particular, in order to keep contact resistance to a minimum, the most substantial and secure connections should be made. The binding posts accept banana plugs, telephone tips, spade lugs, alligator clips, and bare wire. The largest or heaviest mating connection should be made, and, where applicable, the binding posts should be securely tightened.

These considerations may be relaxed whenever single milliohms are considered significant for the task being performed.

3.2.3 Four-Wire Kelvin-Lead Connections

Whenever possible, 4-wire Kelvin leads, the ideal connection, should be employed. Such a connection minimizes the effects of contact resistance and approaches ideal performance.

If the four terminals are available as clamps similar to alligator clips, they may be connected to the necks of the binding posts. If the four terminals are available separately, the optimal connection is shown in Figure 3.1, where the current leads are introduced into the top of the binding posts, and the voltage leads at the necks.

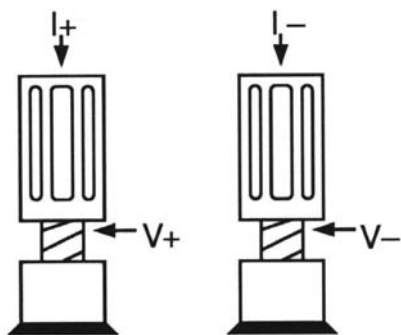


Figure 3.1 Optimal 4-Wire Kelvin Lead Connection

3.2.4 Thermal emf Considerations

The highest-quality low-ernf components are used in the **RX Series**. There nevertheless may be some minute thermal emf generated at the test leads where they contact the gold banana jacks.

This emf will not reflect itself if an ac measurement instrument is employed. It will also be eliminated if a meter with so called “True Ohm” capability is used. Otherwise it may represent itself as a false component of the dc resistance measurement.

3.3 Dial Setting

Whenever the dials are used in positions 0-9, the resulting resistance is simply read directly. Both the decimal point and the steps are clearly marked on the panel.

For additional flexibility and range, each decade provides a “10” position setting. This “10” position on any one decade equals the “1” position on the next higher decade. It adds about 11% to the nominal total decade resistance.

To determine the resistance obtained when one or more “10” settings are used, simply add “1” to the next higher decade. For example, a setting of 3-6-10-0-10 Ω becomes:

3	3	0	0	0	0
6	6	0	0	0	0
10	1	0	0	0	0
0			0	0	
10			1	0	
TOTAL	3	7	0	1	0

and a setting of 10-10-10-10-10.10 Ω becomes:

10	1	0	0	0	0	0.0
10	1	0	0	0	0	0.0
10		1	0	0	0	0.0
10			1	0	0	0.0
10				1	0	0.0
.10						1.0
TOTAL++	1	1	1	1	1	1.0

3.4 Environmental Conditions

For optimal accuracy, the decade box should be used in an environment of 23°C. It should be allowed to stabilize at that temperature after any significant temperature variation.

Humidity should be maintained at laboratory conditions. This is especially important if high resistances are involved.

